


Quick Start Guide



Setup Overview

Refer to your User's Manual for full System instructions and information.

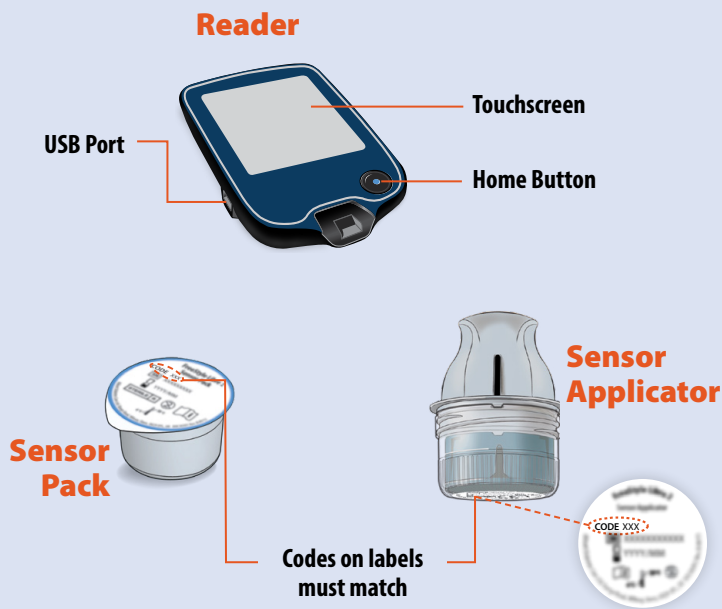


- 1 Assemble and Apply Sensor to your body**
- 2 Start new Sensor with Reader**
Wait 60 minutes for start-up
- 3 Check your glucose whenever you want for up to 14 days**

1 Assemble and Apply Sensor to your body

Get Ready

STEP 1



Select site on back of upper arm.


Note: Avoid scars, moles, stretch marks, lumps and insulin injection sites. To prevent skin irritation, rotate sites between applications. Consider your comfort and activities.

STEP 2



Wash site using a plain soap, dry, and then clean with an alcohol wipe. Allow site to air dry before proceeding.

STEP 3

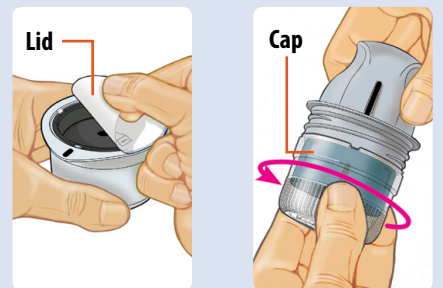


Peel lid completely off Sensor Pack. Unscrew cap from Sensor Applicator.

CAUTION: Sensor codes must match on Sensor Pack and Sensor Applicator.




Prepare Sensor Applicator

STEP 4



Line up dark mark on Sensor Applicator with dark mark on Sensor Pack. On a hard surface, press down firmly on Sensor Applicator until it comes to a stop.

STEP 5



Lift Sensor Applicator out of Sensor Pack.

STEP 6




Sensor Applicator is ready to apply Sensor.

CAUTION: Sensor Applicator now contains a needle. Do not touch inside Sensor Applicator or put it back into Sensor Pack.

Apply Sensor


STEP 7



Place Sensor Applicator over site and push down firmly to apply Sensor.


CAUTION: Do not push down on Sensor Applicator until placed over prepared site to prevent unintended results or injury.

STEP 8



Gently pull Sensor Applicator away from your body.

STEP 9

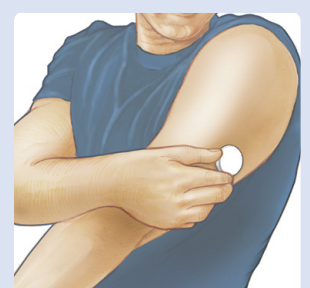

Make sure Sensor is secure. Discard the used Sensor Pack and Sensor Applicator. See *Disposal* section in the User's Manual.




2 Start new Sensor with Reader

STEP 1



Press Home Button to turn on Reader.
Note: If using Reader for the first time, follow the prompts to set date and time.

STEP 2




Touch **Start New Sensor**.

STEP 3




Hold Reader within 4 cm (1.5 inches) of Sensor to scan it.
Sensor can be used to check your glucose after 60 minutes.

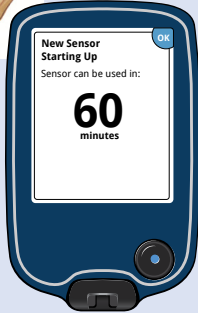

3 Check your glucose

STEP 1



Press Home Button to turn on Reader.

STEP 2




Hold Reader within 4 cm (1.5 inches) of Sensor to scan it.

STEP 3

Message
Touch for more information

Current Glucose
Glucose from your latest scan



Glucose Trend Arrow	What it means
↑	Glucose rising quickly
↗	Glucose rising
→	Glucose changing slowly
↘	Glucose falling
↓	Glucose falling quickly


Reader shows your glucose reading. This includes your Current Glucose, Glucose Trend Arrow, and Glucose Graph.

Setting Alarms


The Sensor automatically communicates with the Reader and can give you glucose alarms if you turn them **ON**. Alarms are **OFF** by default. To turn alarms **ON** or change their settings, follow these steps.

STEP 1



Press Home Button to go to Home Screen. Touch .

STEP 2

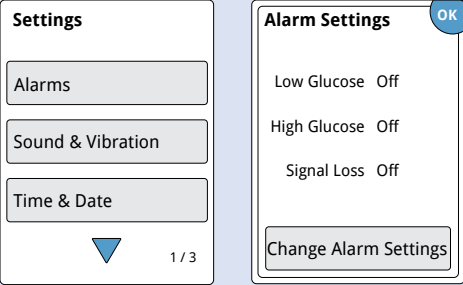

Touch **Alarms** and then touch **Change Alarm Settings**.

STEP 3

Notifies you when glucose is below the level you set.


Notifies you when glucose is above the level you set.

Notifies you when Sensor is not communicating with Reader and that you are not getting Low or High Glucose Alarms.


Select and set your alarms. Touch **done** to save.
Note: The first time you turn on the Low or High Glucose Alarm, the Signal Loss Alarm will automatically turn on too. Touch **Signal Loss Alarm** to turn it off.

Using Alarms



You must scan your Sensor to see your glucose reading.







Touch **Dismiss Alarm & Check Glucose** or press the Home Button to dismiss alarm and check your glucose.

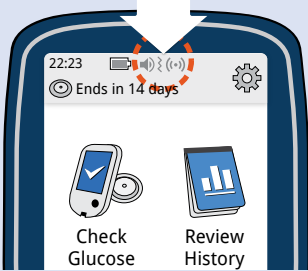

Touch **No** to dismiss alarm.
Touch **Yes** or press the Home Button to dismiss alarm and scan the Sensor.



When any alarm is **ON**, sound/vibration and signal status display on the Home Screen.

Symbol	What it means
	Sound and Vibration ON
	Sound and Vibration OFF
	Sensor communicating with Reader
	Sensor not communicating with Reader

Refer to User's Manual for additional symbols.

If you have followed the instructions described in the User's Manual and are still having difficulty setting up your System or if you are experiencing symptoms that are not consistent with your glucose monitoring, contact your health care professional.

FreeStyle, Libre, and related brand marks are trademarks of Abbott Diabetes Care Inc. in various jurisdictions.
©2019 Abbott ART41106-013 Rev. A 11/19

EC REP

Abbott B.V.
Wegalaan 9, 2132 JD Hoofddorp,
The Netherlands



CE
2797



Abbott Diabetes Care Ltd.
Range Road
Witney, Oxon
OX29 0YL, UK

